

Noninvasive measurement of local temperature using ultrasound-switchable fluorescence: supplement

LIQIN REN,^{1,2}  TINGFENG YAO,^{1,2} KYTAI T. NGUYEN,^{2,3} AND BAOHONG YUAN^{1,2,*}

¹*Ultrasound and Optical Imaging Laboratory, Department of Bioengineering, The University of Texas at Arlington, Arlington, TX 76019, USA*

²*Joint Biomedical Engineering Program, The University of Texas at Arlington and The University of Texas Southwestern Medical Center at Dallas, Dallas, TX 75390, USA*

³*Department of Bioengineering, The University of Texas at Arlington, Arlington, TX 76019, USA*

**baohong@uta.edu*

This supplement published with Optica Publishing Group on 2 August 2023 by The Authors under the terms of the [Creative Commons Attribution 4.0 License](https://creativecommons.org/licenses/by/4.0/) in the format provided by the authors and unedited. Further distribution of this work must maintain attribution to the author(s) and the published article's title, journal citation, and DOI.

Supplement DOI: <https://doi.org/10.6084/m9.figshare.23751033>

Parent Article DOI: <https://doi.org/10.1364/BOE.497815>

NONINVASIVE MEASUREMENT OF LOCAL TEMPERATURE USING ULTRASOUND-SWITCHABLE FLUORESCENCE: SUPPLEMENTAL DOCUMENT

- Fig. S1. IR thermograph (Left) vs. USF image (Right) of $0.99 \times 0.99 \text{ mm}^2$ view at $t_3=0.47 \text{ s}$ when the second peak appears with a background temperature of 36.80°C .

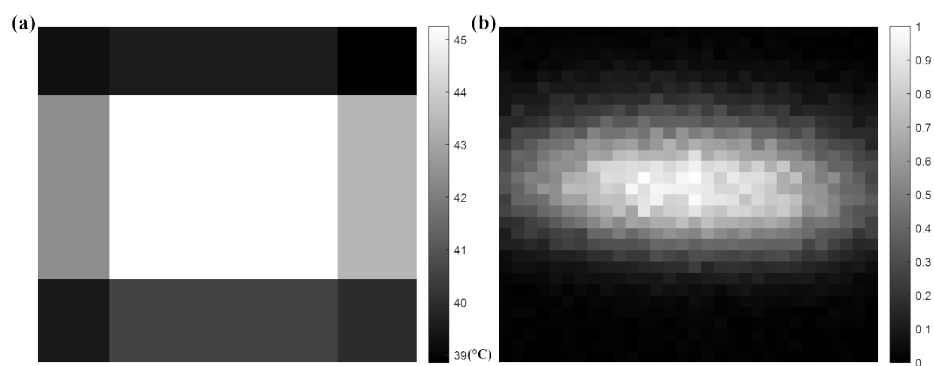


Fig. S1. IR thermograph (Left) vs. USF image (Right) of $0.99 \times 0.99 \text{ mm}^2$ view at $t_3=0.47 \text{ s}$ when the second peak appears with a background temperature of 36.80°C .